



DRILLING PROTOCOL STRAUMANN BLX™/TLX™

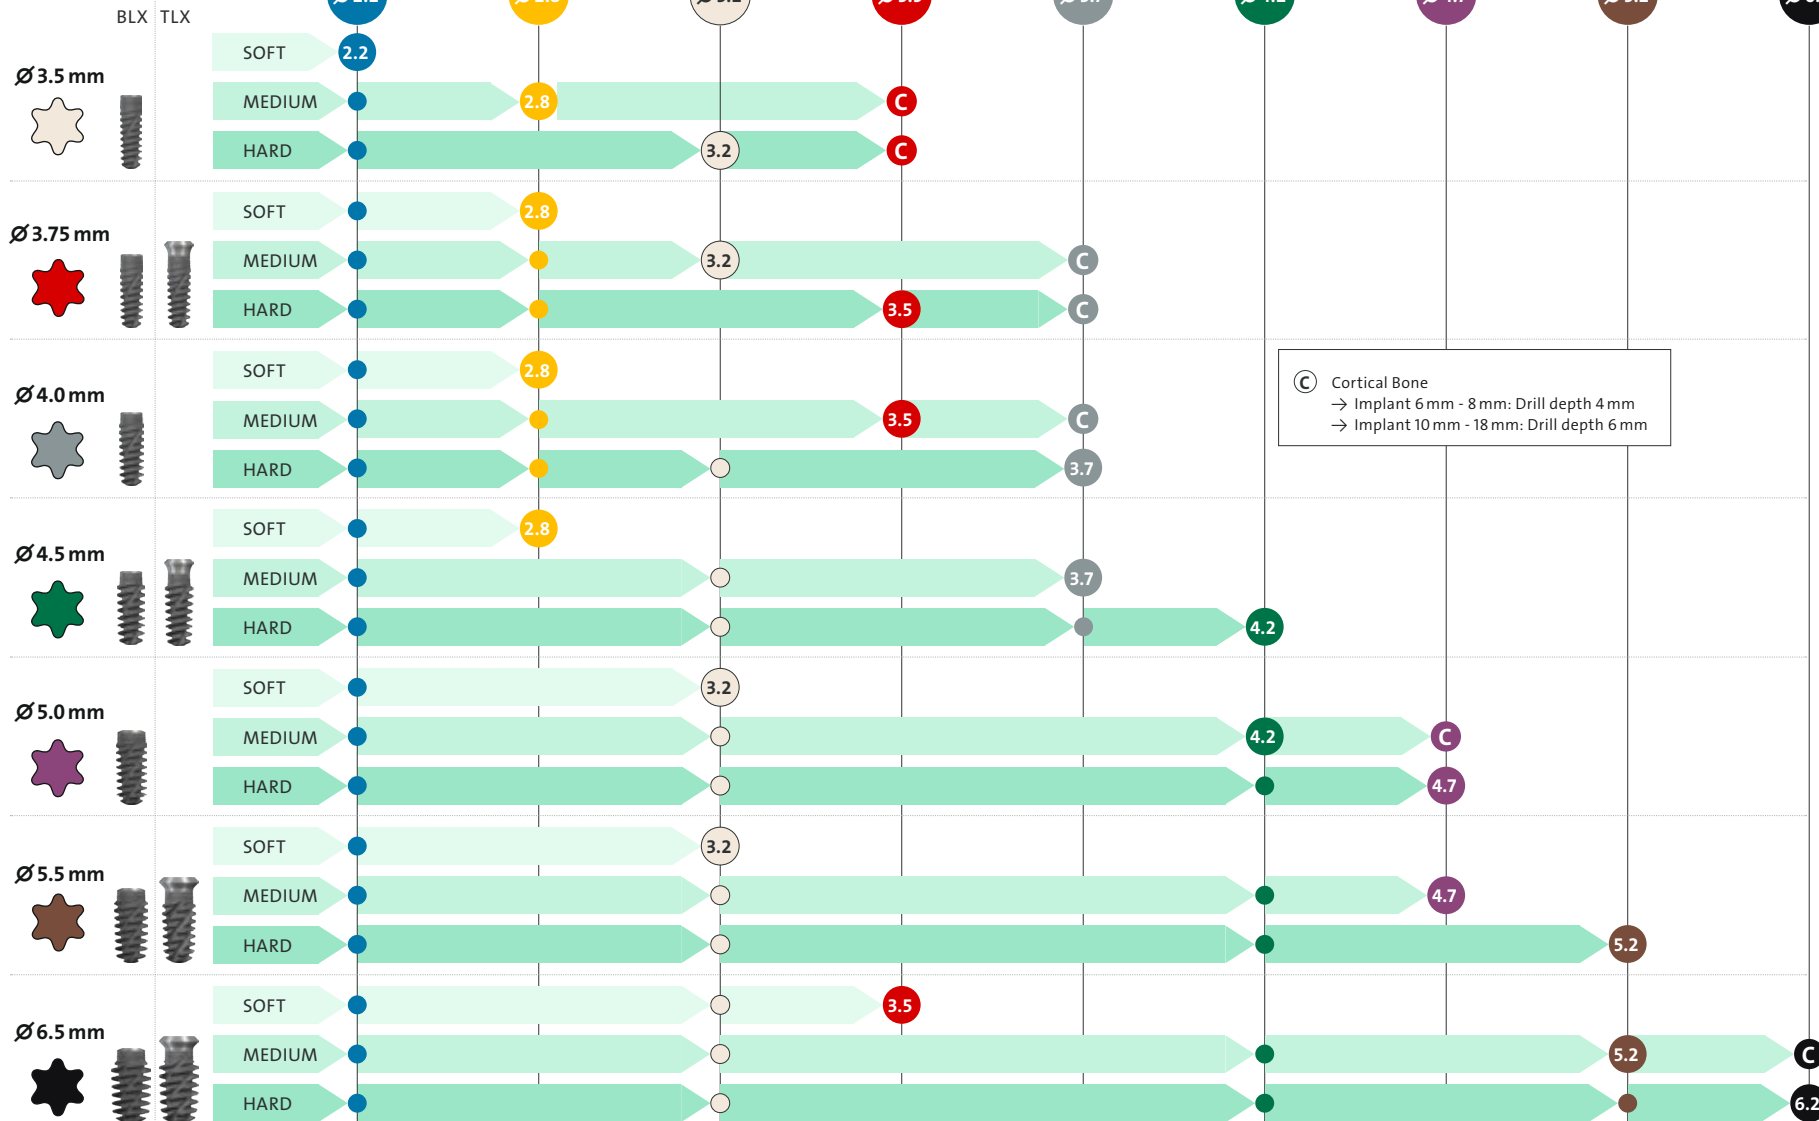

Drilling Protocol Videos

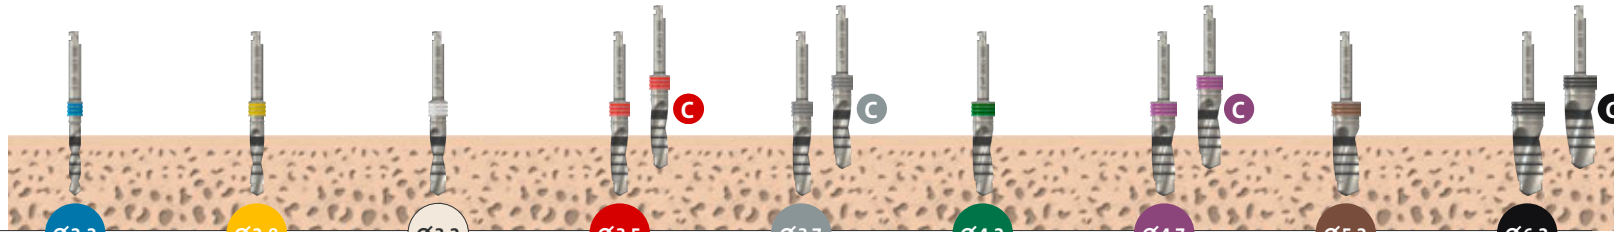

C Cortical Bone
 → Implant 6 mm - 8 mm: Drill depth 4 mm
 → Implant 10 mm - 18 mm: Drill depth 6 mm

International Headquarters
 Institut Straumann AG
 Peter Merian-Weg 12
 CH-4002 Basel, Switzerland
 Phone +41 (0)61 965 11 11
 Fax +41 (0)61 965 11 01
www.straumann.com

© Institut Straumann AG, 2025.
 All rights reserved.
 Straumann® and / or other trademarks and logos from Straumann® mentioned herein are the trademarks or registered trademarks of Straumann Holding AG and / or its affiliates.

041.790/en/E/04 09/25
 707786/en/E/04 09/25